

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17
- 18
- 19
- 20
- 21
- 22
- 23
- 24
- 25
- 26
- 27
- 28

Digital Imaging and Communications in Medicine (DICOM)

Supplement 236: Waveform Presentation State

Prepared by: Working Group 32 Neurophysiology Waveforms

DICOM Standards Committee, Working Group 6

1300 N. 17th Street, Suite 900

Rosslyn, Virginia 22209 USA

Status: Version 30, Aug 23, 2024 – Letter Ballot

Developed pursuant to DICOM Work Item **2022-04B**

29	Table of Contents	
30	Document History.....	3
31	Open Issues	4
32	Closed Issues	4
33	Scope and Field of Application	9
34	Changes to NEMA Standards Publications PS3.3 Digital Imaging and Communications in Medicine	
35	(DICOM) Part 3: Information Object Definitions	10
36	A.1.2.nnn Waveform Presentation State IE	13
37	A.xx Waveform Presentation State Information Object Definitions	13
38	A.xx.1 Waveform Presentation State IOD.....	13
39	A.xx.1.1 Waveform Presentation State IOD Description	13
40	A.xx.1.2 Waveform Presentation State IOD Entity-Relationship Model	13
41	A.xx.1.3 Waveform Presentation State IOD Module Table.....	13
42	A.xx.2 Waveform Acquisition Presentation State IOD	14
43	A.xx.2.1 Waveform Acquisition Presentation State IOD Description	14
44	A.xx.2.2 Waveform Acquisition Presentation State IOD Entity-Relationship Model.....	14
45	A.xx.2.3 Waveform Acquisition Presentation State IOD Module Table.....	14
46	C.xx Waveform Presentation State Modules	15
47	C.xx.hh Waveform Presentation State Relationship Module	15
48	C.xx.aa Structured Waveform Annotation Module.....	17
49	C.xx.bb. Simple Waveform Annotation Module	18
50	C.xx.cc Displayed Waveform Segment Module	19
51	C.xx.dd Montage Activation Module.....	21
52	C.xx.ee Waveform Presentation Montage Module	21
53	C.xx.ff Montage Channel Macro	23
54	C.xx.gg Temporal Range Macro	26
55	C.xx.gg.g Temporal Range Type	27
56	C.xx.gg.h Referenced Sample Position	27
57	F.5.x Waveform Presentation State Directory Record Definition	29
58	Changes to NEMA Standards Publications PS 3.4 Digital Imaging and Communications in Medicine	
59	(DICOM) Part 4: Service Class Specifications	31
60	B.5 Standard SOP classes.....	31
61	Changes to NEMA Standards Publications PS 3.6 Digital Imaging and Communications in Medicine	
62	(DICOM) Part 6: Data Dictionary	31
63	Changes to NEMA Standards Publications PS3.15 Digital Imaging and Communications in Medicine	
64	(DICOM) Part 15: Security and System Management Profiles	34
65	Changes to NEMA Standards Publications PS3.17 Digital Imaging and Communications in Medicine	
66	(DICOM) Part 17: Explanatory Information	36
67	XXX Waveform Presentation (Informative)	36
68		

Document History

2022/06/06	Version 0		Initial version, fragmentary
2022/07/19	Version 1		First draft for wg-32
2022/09/20	Version 5		Draft for wg-06 / First Read
2022/10/14	Version 6		Changes after First Read
2022/11/11	Version 7		Added Cardio Use Case
2022/11/18	Version 8		After Discussion with WG-06
2023/01/18	Version 9		Prepared for WG-06 (2023-01-18)
2023/01/20	Version 10		Changes during and after WG-06 discussion Jan.2023
2023/03/17	Version 11		Prepared for WG-06 (2023-03-20)
2023/03/24	Version 12		Changes during WG-06 discussion (2023-03-20)
2023/03/24	Version 13		Prepared for WG-32 (2023-03-28)
2023/05/17	Version 14		Prepared for WG-32 (2023-05-17) <ul style="list-style-type: none"> • removed Annotation SR, moved to a separate document
2023/06/15	Version 15		Prepared for WG-32 (2023-06-15) <ul style="list-style-type: none"> • removed separate (Non-Patient-related) Montage object, only explicitly defined montages are required
2023/08/23	Version 16		Changes after meeting with WG-06 (June 2023) <ul style="list-style-type: none"> • removed Structured Display IOD and renamed the document • Structured Annotation Module • Montage Activation Module
2023/08/29	Version 17		Prepared for WG-06 (2023-08-30): <ul style="list-style-type: none"> • Presentation State Identification • Additional open issues • PS3.4 and PS3.6 changes
2023/08/29	Version 18		<ul style="list-style-type: none"> • Edits discussed in Meeting with WG-06 (2023-08-30) <ul style="list-style-type: none"> ○ Closed some open issues ○ Move Multiplex Group issues to a separate CP
2024/01/05	Version 19		<ul style="list-style-type: none"> • Document cleaned up • Re-written Open Issue #2
2024/01/12	Version 20		Changes during and after review with WG-06. <ul style="list-style-type: none"> • No authors for individual annotations in the PR – see closed issue #6 • No graphics in the Graphic Annotation Module, just text. Also changed the name of the module. • Removed ICC Profile Module and added an open issue for it (open issue #6). • Removed amendment of PS3.4 and placed an open issue for it (open issue #7) • Cleaned up the comments and preserved the

			discussions in additional closed issues.
2024/03/22	Version 22		Changes during and after Review with WG-06 <ul style="list-style-type: none"> • reworked Instance References (in the PR Relationship Module) • New IOD for Acquisition PR • changed Module Table overview • Changes in the Waveform Presentation State Relationship Module (also contain the reference to the Waveform Annotations SR) and in the Structured Waveform Annotations Module
2024/04/10	Version 23		Prepared for WG-32
2024/05/11	Version 24		Prepared for WG-06 2024-05
2024/05/29	Version 25		Prepared for WG-06 2024-05
2024/05/30	Version 26		Prepared for WG-06 2024-05
2024/05/30	Version 27		Public Comment
2024/08/16	Version 28		public comments, prepared for WG-06 2024-08
2024/08/22	Version 29		Review with WG-06, added new section for changes in PS3.3 F.x
2024/08/23	Version 30		Review with WG-06; prepared for Letter Ballot

70

Open Issues

--	--

71

Closed Issues

1.	<p>Q: Should annotations also be included in the presentation state object or should annotations be saved separately - e.g. in a separate SR document. If both is applicable: a clear distinction criterion is required: which annotations shall go to the display object, which go to the SR document.</p> <p>A: Annotations expressing clinical information (observations, measurements, ...) should go to a separate object, a DICOM SR document.</p>
2.	<p>Q: What sort of time information is required for display relevant information (when a filter was applied, when the montage was changed)? Relative to the recording (ms or samples)?</p> <p>A: relative to the recording</p>
3.	<p>Q: All IODs in PS3.3 A.33 Softcopy Presentation State Information Object Definitions relate to images, intention is the corrected display of pixel values. PS3.4 N describes how these objects apply to images. If the new Waveform Presentation State IOD is added to A.33, PS3.4 N needs to distinguish between different sorts of Softcopy Presentation State objects. Would it be better to add the new IODs in a separate chapter in PS3.3 (e.g. A.xx Waveform Presentation State Object Definitions)?</p> <p>A: Waveform Presentation State IOD has to go to a separate chapter in PS3.3. Description of Storage of these PRs has to go to a separate section in PS3.4.</p>
4.	<p>Q: Procedure Log is a SR intended to store time stamped events during a procedure (e.g. catheterization lab). Would the Procedure Log IOD fit the requirements as well as the</p>

	<p>Presentation State IOD? In imaging Presentation State objects are (usually) created after image creation, the neurophysiology the recording use case requires the PR to be created during the recording.</p> <p>A: Use a separate object to store the annotations, but an SR.</p>
5.	<p>Sup222 Microscopy Bulk Simple Annotations Storage introduced the definition of Annotations as separate IEs in MORW and E-R model. Shall the new IODs make use of this IE or choose another wording (not using Annotation) in order to keep the distinction?</p> <p>A: The existing definition is very general and does not contradict its use for waveforms. In the new IODs introducing the Annotations for waveforms, the definition could be narrowed.</p>
6.	<p>Q: Presentation State Identification contains date/time, when the PR was created, and coded content descriptor and content creator (optional). Is this sufficient to meet legal and billing requirements or should the authorship be stored for every annotation individually?</p> <p>A: Annotations which require authorship have to be stored in the Annotation SR, unless the authorship of the entire PR is sufficient. There is no authorship for individual annotations in the PR.</p>
7.	<p>Q: How should color and shading be encoded in the Presentation State and in the Structured Display Object?</p> <p>A: CIE Lab values</p>
8.	<p>Q: Is there a general requirement to have a temporal assignment of display settings (filters and montages): When where which settings in place? Or is this information just relevant in conjunctions with annotations: which settings were in place when the observations were made.</p> <p>A: The start time for a montage (offset in seconds to the start of the recording) can be stored.</p>
9.	<p>Q: A montage can combine any type of channels from different object types, not just EEG channels from Routine Scalp EEGs. A mechanism is required that provides the information about what type of object the channels belong to.</p> <p>A: The reference to the original waveforms contains both, SOP Instance UID and SOP Class UID.</p>
10.	<p>Q: A concrete Presentation State object contains references to concrete SOP Instances - to concrete objects. It must be guaranteed that this reference works for recordings having been split to multiple files due to limitations on file size or recording gaps.</p> <p>A: Multiple objects can be referenced; multiplex groups can span multiple objects.</p>
11.	<p>Q: Should the Presentation State contain timing information? In a sense: for which time range should this display settings be used. How should viewers then behave? Do they switch the display (the filters, montages) when scrolling through the recording?</p> <p>A: The Waveform Presentation State may contain timing information when (relatively to the recording) a montage was onset. It is up to the display implementers how to use this information.</p>
12.	<p>Does the MORW and the E-R model require an extension by introducing a new IE "Waveform Presentation"?</p>

	A: Yes. Reason is, the current Presentation State IE is image oriented.
13.	<p>Q: Some Modules in the Presentations state allow for (optionally) denoting who added the information (the annotation, the segment of interest). This supplement proposes to use the Attribute Operator's Name and to restrict this to persons. Should also be devices/algorithms possible?</p> <p>A: There is no authorship for individual annotations in the PR – see closed issue #6. On the level of the PR itself, a personal authorship can be expressed via the Content Creator Macro in the Presentations State Identification Module or – if the PR is created by a device - via the General Equipment Module.</p>
14.	<p>Q: Shall Waveform Presentations States have a separate, new Modality Code?</p> <p>If no, the existing Presentation Series Module can be reused. In this case the description there has to be adapted (the Note talks about images).</p> <p>A: No. The new IOD would differ only with respect to this new Modality Code. The existing Module can be reused.</p>
15.	<p>Q: The Presentation State Relationship Module as currently defined can only be used for images (or CDA). It would require comprehensive changes if it should be used for waveforms as well (e.g. for images, it can refer to a list of frames. For waveforms, it has to refer to a list of channels).</p> <p>There were also discussions about cases, where a presentation state would reference both, image objects and waveform objects (e.g. in angiography or in echocardiography). This is reflected in another open issue.</p> <p>A: Under the assumption that Presentation States refer either to images or to waveforms the decision is to use a separate Module instead of changing the existing.</p>
16.	<p>Q: Shall Annotations in the PR use the existing Attribute "Observation DateTime" to reflect the point in time when the annotation was added?</p> <p>A: No. A new Attribute shall be defined. Observation DateTime is only used in SR context.</p>
17.	<p>Q: What are the conditions to record the display montages during waveform acquisition (recording use case)? What information should be stored and which time precision is required?</p> <p>A: There is always a montage defined. The first has to start at the beginning (beginning of the recording). The start times of the different montages shall be in timely order. Time precision "second" is sufficient.</p>
18.	<p>Q: This presentation state object introduces the possibility to assign display properties to waveform annotations coming from separate SR documents. Currently this is constraint to only allow Waveform Annotation SR as a source. Should we expand the scope that such annotations come from SR objects with various SOP Classes?</p> <p>A: No. Annotations from different types of waveforms such as ECG go to the same Waveform Annotation SR object. Annotation Groups are also found in other contexts like Microscopy and there is no intention to expand this presentation state to these objects.</p>
19.	<p>Q: Is it sufficient to just create a single Presentation State to store the display settings (montages) for a neurophysiology study during recording? Are there any other situations which also could trigger to store montage settings and so result in more than one Presentation State in one Study?</p> <p>A: Having more than one PR would not influence the content of the PR IOD. It is up to the</p>

	display application how to present this fact to the user and how to select the PR to present.
20.	<p>Q: Is it sufficient to just create a single Presentation State to store the display settings (montages) for a neurophysiology study during recording? Is there any other situation which also could trigger to store montage settings and so result in more than one Presentation State in one Study?</p> <p>A: Having more than one PR would not influence the content of the PR IOD. It is up to the display application how to present this fact to the user and how to select the PR to present.</p>
21.	<p>Q: Shall it be possible to refer to both – images and waveforms - from one PR, e.g. in Angiography or fMRI? Usually the objects are synchronized, but the existing PR objects only allow for referencing images and the new ones defined in this supplement only allows for referencing waveforms.</p> <p>A: No comments, open issue is closed and the supplement remains as currently done.</p>
22.	<p>Q: Besides the storage of montages used in a neurophysiology recording, the proposed PR allows for both: containing simple text annotations and providing display information for annotations stored in a separate Waveform Annotation SR. Are there any scenarios which require annotations in the PR or shall all annotations go to SRs (there might be different ones depending on the situation when they are created)?</p> <p>A: No comments, open issue is closed and the supplement remains as currently done.</p>
23.	<p>Q: This supplement restricts the Presentation State to only refer to SR documents in the same study. There might be use cases were the annotation SR resides in a different study. Should this be possible in the PR considering, that this results in issues in deciding about which metadata (Study A, Study B) to display?</p> <p>A: No use cases were provided showing the necessity to allow referencing across multiple studies. A note was added to section C.xx.hh describing the fact, that the PR and the SR documents and the waveforms all belong to one study.</p>
24.	<p>Q: Is it necessary to include the ICC Profile Module if all color values are defined as CIE Lab values in PCS?</p> <p>A: No. All Attributes with color information are defined to contain PCS values.</p>
25.	<p>Q: This supplement allows assigning simple text annotations to dedicated waveforms – besides having complex annotations in referenced Waveform Annotation SR documents. Presentation states for images support in addition presentation properties like graphical annotations. Are there any use cases which would require such additional properties in the Waveform Presentation State and, if yes, which one?</p> <p>A: No comments, open issue is closed and the supplement remains as currently done.</p>
26.	<p>Q: Within the presentation state object only the temporal coordinates of the annotation and color properties are defined. All other properties are left to the implementation of the viewing software. Would it be necessary to specify further display properties in the presentation state and, if yes, which one?</p> <p>A: No comments, open issue is closed and the supplement remains as currently done.</p>
27.	<p>Q: Part 4 of the DICOM Standard provides a comprehensive chapter which describes the behavior of applications when they create and assign Presentation States to images (e.g. by a description of the pixel value rendering pipeline).</p> <p>The Waveform Presentation State is not intended to fully render the display of waveforms. Therefore no Service Class specific behavior is described in this supplement. Are there any specific requirements for displays to be normatively defined for applications assigning</p>

	<p>Waveform Presentation States to waveforms and, if yes, which one?</p> <p>A: No comments, open issue is closed and the supplement remains as currently done.</p>
28.	<p>Q: Waveform montages introduced in the supplement are fully defined within the Waveform Presentation State object, that uses them. Montages could also be defined and managed externally. Would it be necessary to also standardize such predefined montages and allow to refer to them in the Waveform Presentation State? If yes, this requires separate mechanisms to address and access such montage objects.</p> <p>A: No comments were received, so this issue is closed for this supplement. It may be addressed later in a separate supplement document, if necessary.</p>
29.	<p>Q: Is there any relevant information missing that should be added to Part 17?</p> <p>A: No comment was received on this, so changes for Part 17 remain unchanged.</p>
30.	<p>Q: Are there any properties in the PR that need to be digitally signed?</p> <p>A: Add the new Modules added in this supplement (C.xx.hh, C.xx.aa, C.xx.bb, C.xx.cc, C.xx.dd, C.xx.ee) to PS 3.15 Section C.2 (end of list of Attributes to be included in the digital signature).</p>
31.	<p>Q: In PC the question was raised that as if Annotation is defined in PS3.3 Section 3.8, annotation should be Annotation (first letter be capitalized)?</p> <p>A: No. Only capitalize, if exactly the defined Annotation from PS3.3 is meant. The definition in PS 3.3 Section 3.8 relates to the IE added for Microscopy Bulk Simple Annotations. The annotations in context of this supplements should not interfere with the specific usage there.</p>
32.	<p>Q: When annotations are added to waveforms the user often sees the recording using a specific montage. Supplement 239 Waveform Annotations and this supplement define Annotations as always referring to the recording channels in the related waveforms but it allows to store a recommended montage to show the annotation.</p> <p>Would it be useful if some annotations could choose to refer to the montage channel(s) instead of the recording channel(s)? For the Annotations stored in a separate SR object the definition of this relationship might be complicated.</p> <p>A: No comments, open issue is closed and the supplement remains as currently done. The Waveform Presentation State just provides a view on the data, the clinical data are in the SR document and in the waveform. There should be no dependency from clinical data to viewing information.</p> <p>If viewing information like the montage would be added to the SR document and later it turns out to be wrong, this would invalidate the SR document, which should be avoided. DICOM does not provide a mechanism to invalidate clinical objects and replace them by other.</p>

73

Scope and Field of Application

74 This supplement introduces Service Classes for storage and exchange of presentation information for
75 DICOM waveform objects by adding Waveform Presentation State IODs. The Waveform Presentation
76 State object stores the display montages, i.e. calculative combinations of recorded channels, display filter
77 settings, and other display properties as well as arbitrary Annotations.

78 This supplement

- 79 • adds a new Waveform Presentation State IE
- 80 • adds new SOP Classes to store Waveform Presentation States and the related Modules
- 81 • amends the Basic Directory IOD by adding Waveform Presentation as a new Directory Type

82

83 In clinical neurophysiology it is important to be able to recreate the presentation of the recorded data as it
84 was displayed during the recording or during review and reporting. This is important for example when
85 activity is noted by the operator during recording and that view needs to be recreated post-hoc for review
86 by a specialist.

87 In cardiology, technicians annotate previously recorded waveforms (e.g. from home monitoring Holter
88 ECG) and highlight areas of interest. This information is essential input for the cardiologist who reviews
89 the ECG and finally provides the report.

90 Waveform objects support limited display information, which has to be provided within the recorded
91 waveforms. These Attributes only cover color and scaling of waveform channels.

92 A **Waveform Presentation State object** provides simple textual annotations, segments of interest,
93 montages including filters, colors, gain, and display scale for a given recording (patient related).

94 In neurophysiology a **montage** defines a list of channels for visualization of the data which is created by a
95 list of original channel sources and the method for their mathematical (linear) recombination.

96 **Waveform annotations** are textual or coded markers assigned to a specific timepoint or time range,
97 related to all channels or a selected set of channels. Annotations could be observations as well as
98 measurements.

99

100
101
102

**Changes to NEMA Standards Publications PS3.3
Digital Imaging and Communications in Medicine (DICOM)
Part 3: Information Object Definitions**

103

104 *Add a new Overview Table to PS3.3 Section A.1.4.:*

105
106

Table A.1-x. Composite Information Object Modules Overview – Waveform Presentation States


IODs Modules	Waveform Presentation State	Waveform Acquisition Presentation State
Patient	M	M
Clinical Trial Subject	U	U
General Study	M	M
Patient Study	U	U
Clinical Trial Study	U	U
General Series	M	M
Clinical Trial Series	U	U
Presn. Series	M	M
Sync.	C	C
General Equip.	M	M
Enhanced General Equip.	M	M
Presn. State Ident.	M	M
Waveform Presn. State Relationship	M	M
Structured Waveform Annotations	U	U
Simple Waveform Annotations	U	U
Displayed Waveform Segments	U	U
Montage Activation	U	M
Waveform Presentation Montage	C	M
SOP Common	M	M

107

108

109 *Amend PS3.3 Figure 7-1.a DICOM Model of the Real World by adding Waveform Presentation State IE*


110

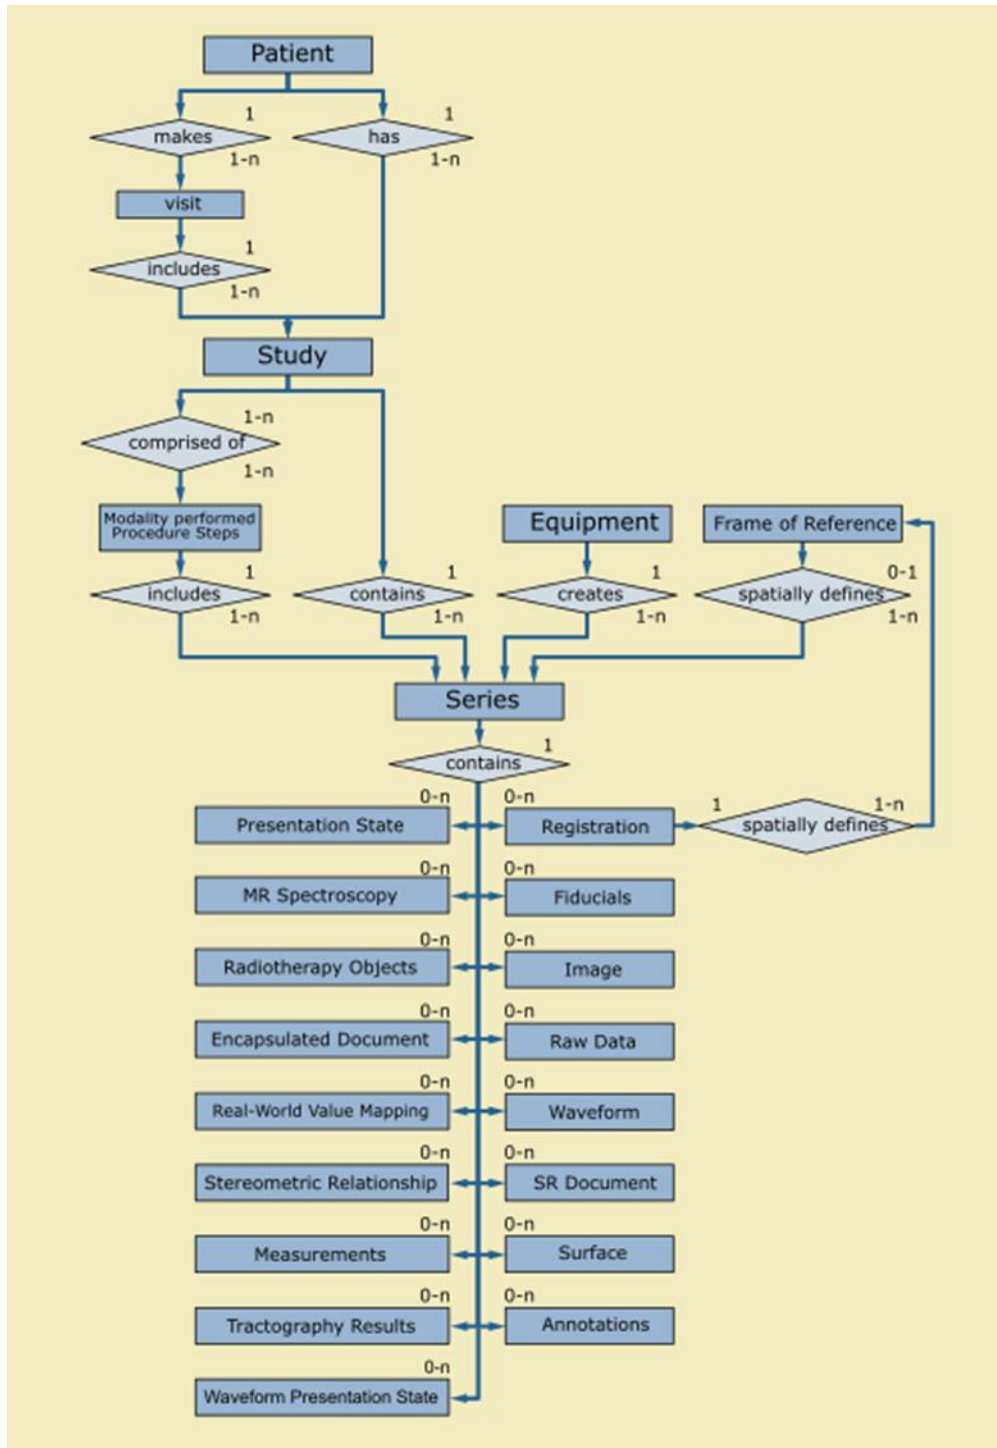

111

112

113 Amend PS3.3 Figure A.1-1 DICOM Composite Instance IOD Information Model by adding the Waveform
 114 Presentation State IE

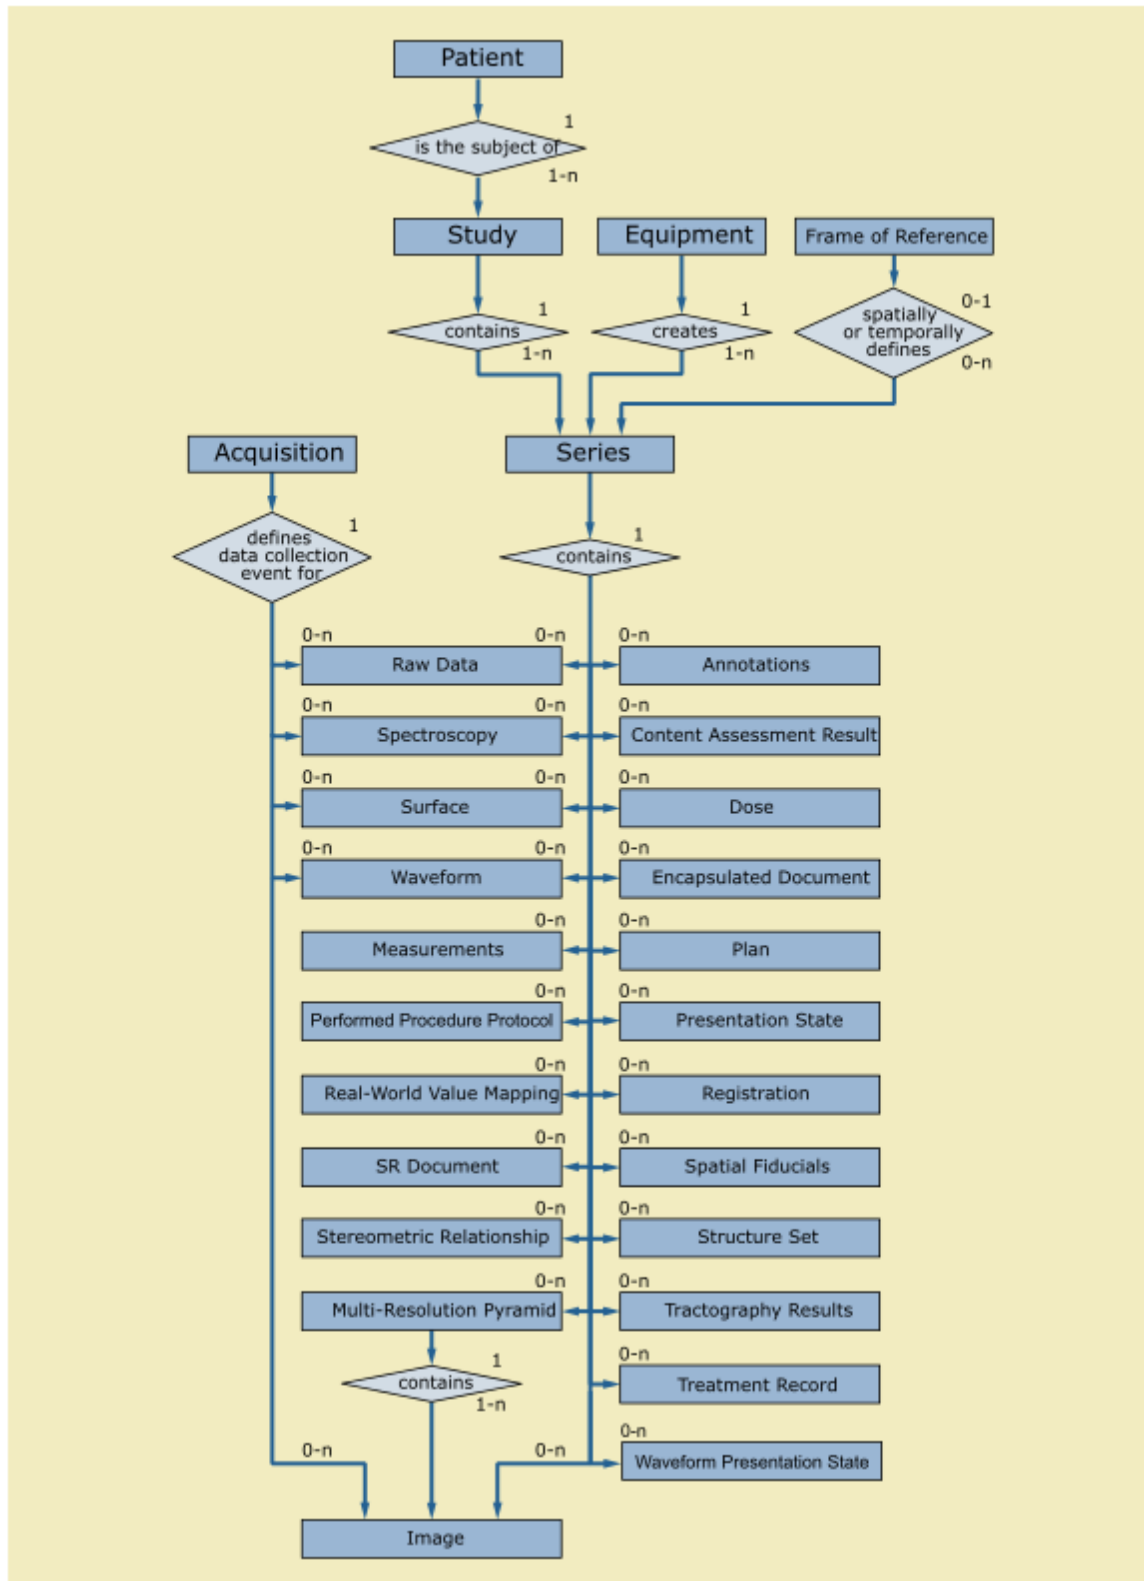

115

116

117 Add the following new content to PS3.3 Section A.1.2.

118 **A.1.2.nnn Waveform Presentation State IE**

119 The Waveform Presentation State IE defines how referenced waveforms will be presented.

120 The Waveform Presentation State IE comprises simple text annotations, segments of interest, and
 121 montages including filters, colors, gain, and vertical sizes of waveform channels if this information is to be
 122 applied to the referenced waveform(s). It might also contain display information for structured annotations
 123 related to the referenced waveform(s).

124

125 *Add the following new content to PS3.3 Section A.xx*

126 **A.xx Waveform Presentation State Information Object Definitions**

127 **A.xx.1 Waveform Presentation State IOD**

128 **A.xx.1.1 Waveform Presentation State IOD Description**

129 The Waveform Presentation State Information Object Definition (IOD) specifies information that may be
 130 used to present (display) waveforms that are referenced from within the IOD.

131 Note: The Waveform Presentation State object allows to store simple textual annotations, as well as to provide
 132 display information for annotations stored in a separate SR document. The policies related to the criteria
 133 for where specific annotations should be stored – in the Waveform Presentation State object or in the
 134 SR document – are outside the scope of the Standard.

135 **A.xx.1.2 Waveform Presentation State IOD Entity-Relationship Model**

136 This IOD uses the E-R Model in Section A.1-2, with only the Waveform Presentation State IE below the
 137 Series IE.

138 **A.xx.1.3 Waveform Presentation State IOD Module Table**

139 Table A.xx.1-1 specifies the Modules of the Waveform Presentation State IOD.

140 **Table A.xx.1-1. Waveform Presentation State IOD Modules**

IE	Module	Reference	Usage
Patient	Patient	C.7.1.1	M
	Clinical Trial Subject	C.7.1.3	U
Study	General Study	C.7.2.1	M
	Patient Study	C.7.2.2	U
	Clinical Trial Study	C.7.2.3	U
Series	General Series	C.7.3.1	M
	Clinical Trial Series	C.7.3.2	U
	Presentation Series	C.11.9	M
Frame of Reference	Synchronization	C.7.4.2	C – Required if time synchronization was applied.
Equipment	General Equipment	C.7.5.1	M
	Enhanced General Equipment	C.7.5.2	M
Waveform Presentation State	Presentation State Identification	C.11.10	M
	Waveform Presentation State Relationship	C.xx.hh	M
	Structured Waveform Annotation	C.xx.aa	U

	Simple Waveform Annotation	C.xx.bb	U
	Displayed Waveform Segment	C.xx.cc	U
	Montage Activation	C.xx.dd	U
	Waveform Presentation Montage	C.xx.ee	C – Required if Montage Activation Module is present.
	SOP Common	C.12.1	M

141

142

143

144

Note: All Attributes containing color information are defined to contain PCS values, so the ICC Profile Module is not used.

145 A.xx.2 Waveform Acquisition Presentation State IOD

146 A.xx.2.1 Waveform Acquisition Presentation State IOD Description

147 The Waveform Acquisition Presentation State Information Object Definition (IOD) provides information
148 about the display settings like filters and montages used during acquisition of the waveform. This allows
149 presentation of the “recording view” later during review of the waveform.

150

151

152

153

154

Note: The Presentation State object allows to store simple textual annotations, as well as to provide display information for annotations stored in a separate SR document. The policies related to the criteria for where specific annotations should be stored – in the Presentation State object or in the SR document – are outside the scope of the Standard.

155 A.xx.2.2 Waveform Acquisition Presentation State IOD Entity-Relationship Model

156 This IOD uses the E-R Model in Section A.1-2, with only the Waveform Presentation State IE below the
157 Series IE.

158 A.xx.2.3 Waveform Acquisition Presentation State IOD Module Table

159 Table A.xx.2-1 specifies the Modules of the Waveform Acquisition Presentation State IOD.

160

Table A.xx.2-1. Waveform Acquisition Presentation State IOD Modules

IE	Module	Reference	Usage
Patient	Patient	C.7.1.1	M
	Clinical Trial Subject	C.7.1.3	U
Study	General Study	C.7.2.1	M
	Patient Study	C.7.2.2	U
	Clinical Trial Study	C.7.2.3	U
Series	General Series	C.7.3.1	M
	Clinical Trial Series	C.7.3.2	U
	Presentation Series	C.11.9	M
Frame of Reference	Synchronization	C.7.4.2	C – Required if time synchronization was applied.
Equipment	General Equipment	C.7.5.1	M
	Enhanced General Equipment	C.7.5.2	M
Waveform Presentation State	Presentation State Identification	C.11.10	M
	Waveform Presentation State	C.xx.hh	M

	Relationship		
	Structured Waveform Annotation	C.xx.aa	U
	Simple Waveform Annotation	C.xx.bb	U
	Displayed Waveform Segment	C.xx.cc	U
	Montage Activation	C.xx.dd	M
	Waveform Presentation Montage	C.xx.ee	M
	SOP Common	C.12.1	M

161

162 Note: All Attributes in this IOD containing color information are defined to contain PCS values, so the ICC Profile
163 Module is not used.

164

165 *Adapt Section PS3.3 Section C.10.10.1 by adding an additional note to indicate, that this Attribute is also*
166 *used in context of Waveform Presentation States.*

167 **Note 1:**

168 As an example, an annotation that applies to the entire first multiplex group and channels 2 and 3 of the third
169 multiplex group would have Referenced Channels value 0001 0000 0003 0002 0003 0003.

170 **Note 2:**

171 **This Attribute is also used in context of Waveform Presentation States to express the relationship of a**
172 **presentation property to selected waveform channels.**

173

174 *Adapt Section PS3.3 Section C.11.9 by changing the note to reflect, that a PR could not only apply to*
175 *images.*

176 Note

177 This implies that presentation states will be in different Series from the **images instances** to which they apply,
178 which will have different values for Modality.

179

180 *Add the following new content to PS3.3 Section C.xx*

181 C.xx Waveform Presentation State Modules

182 C.xx.hh Waveform Presentation State Relationship Module

183 Table C.xx.hh-1 specifies the Attributes of the Waveform Presentation State Relationship Module, which
184 describes the waveforms to which a Waveform Presentation State applies.

185

186 Note: This module only allows for referencing waveforms and SR documents from a single study. The
187 Presentation State itself will belong to the same study. Creating annotations that reference waveforms
188 and SR documents in a different study can be done by creating another Waveform Presentation State in
189 that other study.

190

191

Table C.xx.hh-1. Waveform Presentation State Relationship Module

Attribute Name	Tag	Type	Attribute Description
Referenced Series Sequence	(0008,1115)	1	Sequence of Items where each Item includes the Attributes of one Series to

Attribute Name	Tag	Type	Attribute Description
			<p>which the Waveform Presentation State applies.</p> <p>One or more Items shall be included in this Sequence.</p>
>Series Instance UID	(0020,000E)	1	<p>Unique identifier of a Series that is part of the Study defined by the Study Instance UID (0020,000D) in the enclosing data set.</p> <p>Note</p> <p>The Study Instance UID (0020,000D) value will be that of the Waveform Presentation State.</p>
>Referenced Instance Sequence	(0008,114A)	1C	<p>The set of SR documents containing waveform Annotations to which the Presentation State applies.</p> <p>These shall be of the Study defined by Study Instance UID (0020,000D) and the Series defined by Series Instance UID (0020,000E).</p> <p>The referenced Instances shall be of SOP Class 1.2.840.10008.5.1.4.1.1.88.77 Waveform Annotation SR Storage.</p> <p>One or more Items shall be included in this Sequence.</p> <p>Required if Structured Waveform Annotation Sequence (ggga,eee1) is present.</p>
>> <i>Include Table 10-11 "SOP Instance Reference Macro Attributes"</i>			
>Referenced Waveform Sequence	(0008,113A)	1	<p>The set of waveforms to which the Presentation State applies. These shall be of the Study defined by Study Instance UID (0020,000D) and the Series defined by Series Instance UID (0020,000E).</p> <p>One or more Items shall be included in this Sequence.</p> <p>The referenced SOP Class shall be the same for all SOP Instances in a single Item of this Referenced Series Sequence (0008,1115) but may be different for different Items.</p> <p>Notes:</p> <ol style="list-style-type: none"> 1. For example, some Series might represent EEG and some Series might represent ECG. 2. The Waveform Presentation State applies to waveforms that are referenced in annotations in Structured Waveform Annotation Sequence (ggga,eee1), thus those waveforms

Attribute Name	Tag	Type	Attribute Description
			also need to be included here.
>>Include Table 10-11 "SOP Instance Reference Macro Attributes"			
>>Referenced Waveform Channels	(0040,A0B0)	1C	Identifies the waveform multiplex group (M) and channel (C) within the referenced waveform SOP Instance using pairs of values (M,C). See Section C.10.10.1.1. Required if the Referenced Waveform SOP Instance contains multiple channels and the reference does not apply to all channels of all multiplex groups.

192

193

194 **C.xx.aa Structured Waveform Annotation Module**

195 This Module defines how a display device applies waveform annotations that are stored in a separate SR
196 document to a waveform.

197

Table C.xx.-aa. Structured Waveform Annotation Module Attributes

Attribute Name	Tag	Type	Attribute Description
Structured Waveform Annotation Sequence	(ggga,eee1)	1	Selects and provides display information for waveform annotations and measurements contained in the referenced SR document. One or more Items shall be included in this Sequence.
>Include Table 10-11 "SOP Instance Reference Macro Attributes"			This references an SR document which contains the annotations. The Instance referenced here shall be contained in the Referenced Instance Sequence (0008,114A) in the Referenced Series Sequence (0008,1115).
>Waveform Annotation Display Selection Sequence	(ggga,eee2)	3	Selects subsets of annotations in the referenced SR document for display. If no subset is selected (i.e. this Attribute is missing or the Sequence is empty) all annotations in the referenced SR document shall be displayed. One or more Items may be included in this Sequence.
>>Annotation Group Number	(0040,A180)	1	References an annotation group number (130872, DCM, "Waveform Annotation Group Number") defined within the referenced SR document to which the display information applies.
>>Referenced Montage Index	(ggga,eeec)	3	The recommended viewing montage

Attribute Name	Tag	Type	Attribute Description
			identified by the Montage Index (ggge,eeee) in the Waveform Montages Sequence (ggge,eeea).
>>Text Color CIELab Value	(0070,0241)	3	A default color triplet value used to specify the text color in which it is recommended that the text be rendered on a color display. The units are specified in PCS-Values, and the value is encoded as CIELab. See Section C.10.7.1.1.

198

199 **C.xx.bb. Simple Waveform Annotation Module**

200 This Module defines Attributes of textual annotations that shall be made available by a display device to
 201 be applied to a waveform. The text is defined in position relative to the waveform time information.

202 A simple waveform Annotation shall be related to a waveform.

203 **Table C.xx.-bb. Simple Waveform Annotation Module Attributes**

Attribute Name	Tag	Type	Attribute Description
Waveform Annotation Sequence	(gggb,eee1)	1	Selects and provides simple textual annotations for a group of waveforms or channels within these waveforms. One or more Items shall be included in this Sequence.
>Annotation DateTime	(gggb,eee2)	3	The date and time the annotation was added.
>Referenced Waveform Sequence	(0008,113A)	1C	The waveform to which this annotation applies. All waveforms referenced here shall be present in Referenced Waveform Sequence (0008,113A) inside the Referenced Series Sequence (0008,1115) in the top-level data set. One or more Items shall be included in this Sequence. Required if the annotation in this Item does not apply to all the waveforms and channels listed in Referenced Waveform Sequence (0008,113A) inside the Referenced Series Sequence (0008,1115) in the top-level data set.
>>Include Table 10-11 "SOP Instance Reference Macro Attributes"			
>>Referenced Waveform Channels	(0040,A0B0)	1	Identifies the waveform multiplex group (M) and channels (C) within the referenced SOP Instance

Attribute Name	Tag	Type	Attribute Description
			using pairs of values (M,C). See Section C.10.10.1.1.
>Include Table C.xx-a "Temporal Range Macro Attributes"			Enumerated Values for Temporal Range Type (0040,A130): POINT MULTIPOINT
>Referenced Montage Index	(ggga,eeec)	3	The recommended viewing montage identified by the Montage Index (ggge,eeee) in the Waveform Montages Sequence (ggge,eeee).
>Text Object Sequence	(0070,0003)	1	Describes a text annotation. A single Item shall be included in this Sequence.
>>Unformatted Text Value	(0070,0006)	1	The text to be displayed.
>>Text Color CIELab Value	(0070,0241)	3	A default color triplet value used to specify the text color in which it is recommended that the text be rendered on a color display. The units are specified in PCS-Values, and the value is encoded as CIELab. See Section C.10.7.1.1.

204

205 **C.xx.cc Displayed Waveform Segment Module**

206 This Module defines Attributes required to define waveform segments and the properties how to display
207 them. A waveform segment is a temporal portion of a waveform ("segment of interest").

208 **Table C.xx-cc. Displayed Waveform Segment Module Attributes**

Attribute Name	Tag	Type	Attribute Description
Displayed Waveform Segment Sequence	(gggc,eee1)	1	Selects and provides display parameters for segments from a group of waveforms or channels within these waveforms. One or more Items shall be included in this Sequence.
>Segment Definition DateTime	(gggc,eee2)	3	The date and time the segment was defined.
>Referenced Waveform Sequence	(0008,113A)	1C	The waveforms to which the segment display parameters in this Item apply. All waveforms referenced here shall be present in Referenced Waveform Sequence (0008,113A) inside the Referenced Series Sequence (0008,1115) in the top-level data set.

Attribute Name	Tag	Type	Attribute Description
			<p>One or more Items shall be included in this Sequence.</p> <p>Required if the segment display parameters in this Item do not apply to all the waveforms and channels listed in Referenced Waveform Sequence (0008,113A) inside the Referenced Series Sequence (0008,1115) in the top-level data set.</p>
>>Include Table 10-11 "SOP Instance Reference Macro Attributes"			
>>Referenced Waveform Channels	(0040,A0B0)	1	<p>Identifies the waveform multiplex group (M) and channels (C) within the referenced SOP Instances using pairs of values (M,C). See Section C.10.10.1.1.</p>
>Include Table C.xx-a "Temporal Range Macro Attributes"			<p>Enumerated Values for Temporal Range Type (0040,A130):</p> <p>SEGMENT</p> <p>MULTISEGMENT</p> <p>BEGIN</p> <p>END</p>
>Waveform Display Background CIELab Value	(003A,0231)	1C	<p>A color triplet value recommended for rendering the waveform display background on a color display. The units are specified in PCS-Values, and the value is encoded as CIELab. See Section C.10.7.1.1.</p> <p>At least one of Waveform Display Background CIELab Value (003A,0231) and Channel Recommended Display CIELab Value (003A,0244) shall be present.</p>
>Channel Recommended Display CIELab Value	(003A,0244)	1C	<p>A color triplet value recommended for rendering the channel on a color display. The units are specified in PCS-Values, and the value is encoded as CIELab. See Section C.10.7.1.1.</p> <p>At least one of Waveform Display Background CIELab Value (003A,0231) and Channel Recommended Display CIELab Value (003A,0244) shall be present.</p>

210 **C.xx.dd Montage Activation Module**

211 This Module defines Attributes recording the timepoints of montage activation.

212 **Table C.xx-dd. Montage Activation Module Attributes**

Attribute Name	Tag	Type	Attribute Description
Montage Activation Sequence	(gggd,eeea)	1	Provides information about when a montage was activated. One or more Items shall be included in this Sequence. The Items shall be ordered by ascending Montage Activation Time Offset (gggd,eeeb) value.
>Referenced Montage Index	(ggga,eeec)	1	The Montage Index (ggge,eeee) of the montage in the Waveform Montages Sequence (ggge,eeee).
>Montage Activation Time Offset	(gggd,eeeb)	1	Time offset in seconds relative to the beginning of the recording. The offset of the first Item shall be 0.

213

214 **C.xx.ee Waveform Presentation Montage Module**

215 This Module contains Attributes describing presentation montages of waveform channels.

216 **Table C.xx-ee Waveform Presentation Montage Module Attributes**

Attribute Name	Tag	Type	Description
Waveform Montage Sequence	(ggge,eeee)	1	Description of the waveform montage(s) in the Waveform Presentation State. One or more Items shall be included in this Sequence.
>Montage Name	(ggge,eeec)	3	The name of the montage.
>Montage Index	(ggge,eeee)	1	The index of the montage within this Sequence. The value shall start at 1 and increase monotonically by 1. This index will be used elsewhere to refer to this specific montage Sequence Item.
>Montage Channel Sequence	(ggge,eeed)	1	The channel(s) that comprise this montage. One or more Items shall be included in this Sequence. The order of Items in this Sequence is significant.
>>Include Table C.xx.-b "Montage Channel Macro Attributes"			
>Waveform Data Display Scale	(003A,0230)	3	The recommended time-based waveform data display scale in units of mm/s (see Section C.10.9.1.8). Note: This does not prevent applications to

			change this during display. The value might be used as an initial default setting.
>Waveform Display Background CIELab Value	(003A,0231)	3	A color triplet value recommended for rendering the waveform display background on a color display. The units are specified in PCS-Values, and the value is encoded as CIELab. See Section C.10.7.1.1.
>Waveform Presentation Group Sequence	(003A,0240)	3	Sequence of Items, each Item describing a Presentation Group of one or more waveform channels to be displayed together. Note A Presentation Group is conventionally denoted a "display page", and a waveform object may be rendered using several Presentation Groups under user display control. One or more Items are shall be included in this Sequence.
>>Presentation Group Number	(003A,0241)	1	A number that identifies the Presentation Group.
>>Channel Display Sequence	(003A,0242)	1	Sequence of Items, each Item describing a channel to be displayed in the Presentation Group. One or more Items shall be included in this Sequence.
>>>Referenced Montage Channel Number	(ggge,eeeb)	1	Number of the montage channel to be displayed in the Presentation Group. This is the ordinal number of the Item in the Montage Channel Sequence (ggge,eed).
>>>Channel Offset	(003A,0218)	3	The offset in seconds from the beginning of the montage channel waveform data to the first sample to be used for presentation. Value may be negative.
>>>Channel Recommended Display CIELab Value	(003A,0244)	1	A color triplet value recommended for rendering the channel on a color display. The units are specified in PCS-Values, and the value is encoded as CIELab. See Section C.10.7.1.1.
>>>Channel Position	(003A,0245)	1	Position of the channel within the Presentation Group display area (see Section C.10.9.1.9).
>>>Display Shading Flag	(003A,0246)	3	Specifies display area shading between the displayed waveform channel and another line. The nature of the shading (e.g., solid, or cross-hatching) is implementation dependent. Enumerated Values: NONE no shading

			<p>BASELINE shading between the waveform and the channel display baseline (sample value 0 equivalent location)</p> <p>ABSOLUTE shading between the waveform and the channel real world actual value 0 (i.e., taking into account the Channel Baseline (003A,0213) value)</p> <p>DIFFERENCE shading between the waveform and a second waveform in the Presentation Group at the same channel position that also has Display Shading Flag (003A,0246) value DIFFERENCE.</p>
>>>Fractional Channel Display Scale	(003A,0247)	1C	Fraction of the Presentation Group vertical display dimension assigned to the unit quantity (least significant bit) of the channel samples (see Section C.10.9.1.10). Required if Absolute Channel Display Scale (003A,0248) is not present, may be present otherwise.
>>>Absolute Channel Display Scale	(003A,0248)	1C	Nominal vertical display height in mm assigned to the unit quantity (least significant bit) of the channel samples (see Section C.10.9.1.10). Required if Fractional Channel Display Scale (003A,0247) is not present, may be present otherwise.

217

218

219 **C.xx.ff Montage Channel Macro**

220 This Macro consists of Attributes describing a single channel of a waveform montage.

221

Table C.xx-b. Montage Channel Macro Attributes

Attribute Name	Tag	Type	Description
Montage Channel Number	(gggf,0202)	1	The number of the montage channel.
Montage Channel Label	(gggf,0203)	3	Text label of the channel, which may be used for display purposes.
Montage Channel Source Sequence	(gggf,0208)	1C	<p>A coded descriptor of the waveform channel source. This identifies a single channel in the recorded waveform in terms of the lead from which it is collected.</p> <p>Required if Source Waveform Sequence (003A,020A) is not present.</p> <p>Only a single Item shall be included in this Sequence.</p>

<i>>Include Table 8.8-1 "Code Sequence Macro Attributes"</i>			<i>DCID 3001 "ECG Leads"</i> <i>DCID 3004 "Arterial Pulse Waveform"</i> <i>DCID 3005 "Respiration Waveform"</i> <i>DCID 3030 "EEG Leads"</i> <i>DCID 3031 "Lead Location Near or in Muscle"</i> <i>DCID 3032 "Lead Location Near Peripheral Nerve"</i> <i>DCID 3033 "EOG Lead"</i> <i>DCID 3034 "Body Position Waveform"</i>
Source Waveform Sequence	(003A,020A)	1C	<p>A Sequence that provides reference to a waveform from which this channel was derived.</p> <p>Required if Montage Channel Source Sequence (gggf,0208) is not present.</p> <p>One or more Items shall be included in this Sequence.</p> <p>If there are multiple Items in this Sequence, they shall share the same multiplex group identified by Multiplex Group UID (003A,0310).</p>
<i>Include Table 10-11 "SOP Instance Reference Macro Attributes"</i>			
>Referenced Waveform Channels	(0040,A0B0)	1	<p>Identifies the waveform multiplex group (M) and channel (C) within the referenced SOP Instances using a pair of values (M,C). See Section C.10.10.1.1.</p> <p>Only a single channel shall be referenced.</p>
Channel Derivation Description	(003A,020C)	3	Additional description of the channel derivation.
Contributing Channel Sources Sequence	(gggf,0209)	2	<p>A Sequence of Items each representing the source of a channel contributing to this montage.</p> <p>Zero or more Items shall be included in this Sequence.</p>
>Channel Weight	(gggf,020A)	1	<p>The relative weight this channel contributes to the montage channel.</p> <p>The weights of all Items in this Sequence shall sum up to 1.</p>
>Channel Source Sequence	(003A,0208)	1C	<p>A coded descriptor of the contributing waveform channel source.</p> <p>Only a single Item shall be included in this Sequence.</p>
<i>>>Include Table 8.8-1 "Code Sequence Macro Attributes"</i>			<i>DCID 3001 "ECG Leads"</i> <i>DCID 3004 "Arterial Pulse Waveform"</i> <i>DCID 3005 "Respiration Waveform"</i> <i>DCID 3030 "EEG Leads"</i> <i>DCID 3031 "Lead Location Near or in Muscle"</i>

			<p><i>DCID 3032 "Lead Location Near Peripheral Nerve"</i></p> <p><i>DCID 3033 "EOG Lead"</i></p> <p><i>DCID 3034 "Body Position Waveform"</i></p>
>Source Waveform Sequence	(003A,020A)	1C	<p>Reference to waveforms from which this channel was derived.</p> <p>One or more Items shall be included in this Sequence.</p> <p>If there are multiple Items in this Sequence, they shall share the same multiplex group identified by Multiplex Group UID (003A,0310).</p>
<i>>>Include Table 10-11 "SOP Instance Reference Macro Attributes"</i>			
>Referenced Waveform Channels	(0040,A0B0)	1	<p>Identifies the waveform multiplex group (M) and channel (C) within the referenced SOP Instance using a pair of values (M,C). See Section C.10.10.1.1.</p> <p>Only a single channel shall be referenced here.</p>
Channel Sensitivity	(003A,0210)	1C	<p>Nominal numeric value of unit quantity of sample. See Section C.10.9.1.4.2.</p> <p>Required if samples represent defined (not arbitrary) units.</p>
Channel Sensitivity Units Sequence	(003A,0211)	1C	<p>A coded descriptor of the units of measure for the Channel Sensitivity (003A,0210). See Section C.10.9.1.4.2.</p> <p>Only a single Item shall be included in this Sequence.</p> <p>Required if Channel Sensitivity (003A,0210) is present.</p>
<i>>Include Table 8.8-1 "Code Sequence Macro Attributes"</i>			<i>DCID 82 "Measurement Unit"</i>
Channel Sensitivity Correction Factor	(003A,0212)	1C	<p>Multiplier to be applied to encoded sample values to match units specified in Channel Sensitivity (003A,0210) (e.g., based on calibration data). See Section C.10.9.1.4.2.</p> <p>Required if Channel Sensitivity (003A,0210) is present.</p>
Filter Low Frequency Characteristics Sequence	(003A,0318)	1C	<p>The properties of low frequency (high-pass) filters applied to the waveform montage channel.</p> <p>Required if a high-pass filter is used.</p>
<i>>Include Table C.10.12-1 "Waveform Filter Characteristics Macro Attributes"</i>			
Filter High Frequency Characteristics Sequence	(003A,0219)	1C	<p>The properties of high frequency (low-pass) filters applied to the waveform montage channel.</p>

			Required if a low-pass filter is used.
>Include Table C.10.12-1 "Waveform Filter Characteristics Macro Attributes"			
Notch Filter Characteristics Sequence	(003A,0321)	3	The properties of notch filters applied to the waveform montage channel.
>Include Table C.10.12-1 "Waveform Filter Characteristics Macro Attributes"			

222

223 **C.xx.gg Temporal Range Macro**224 *Ed. Note: This Macro could also replace this set of Attributes in the Waveform Annotation Module C.10.10*

225 This macro contains Attributes that define one or more points in time or time ranges in waveforms or
 226 dedicated channels of those waveforms. The waveforms and channels are selected in the enclosing data
 227 set.

228 **Table C.xx-a. Temporal Range Macro Attributes**

Attribute Name	Tag	Type	Description
Temporal Range Type	(0040,A130)	1	See Section C.xx.gg.g for Enumerated Values.
Referenced Sample Positions	(0040,A132)	1C	List of samples within a multiplex group specifying one or more temporal points. Position of first sample is 1. See Section C.xx.gg.h. Required if Referenced Time Offsets (0040,A138) and Referenced DateTime (0040,A13A) are not present.
Referenced Time Offsets	(0040,A138)	1C	List of time offsets by number of seconds after start defining one or more temporal points. Required if Referenced Sample Positions (0040,A132) and Referenced DateTime (0040,A13A) are not present.
Referenced DateTime	(0040,A13A)	1C	List of one or more temporal points by absolute datetime. Required if Referenced Sample Position (0040,A132) and Referenced Time Offsets (0040,A138) are not present.

229

230 **C.xx.gg.g Temporal Range Type**

231 *Ed. Note: This is a rewording of existing C.10.10.1.2. In the current Standard this section only belongs to*
 232 *the Waveform Annotation Module*

233 The Temporal Range Type (0040,A130) Attribute defines the type of temporal extent of ~~the annotated~~
 234 ~~region of interest~~ **a selected region of waveform data**. A temporal point (or instant of time) may be
 235 defined by a waveform sample offset (for a single waveform multiplex group only), time offset, or absolute
 236 time.

237 **The value or the values shall be present either as Referenced Sample Positions (0040, A132), or as**
 238 **Referenced Time Offsets (0040,A138), or as Referenced DateTimes (0040,A13A).**

239
 240 Enumerated Values:

241 **POINT** a single temporal point; **a single value shall be present.**

242 **MULTIPOINT** multiple temporal points; **multiple values shall be present.**

243 **SEGMENT** a range between two **different** temporal points; **two values shall be present.**

244 **MULTISEGMENT** multiple segments, each denoted by two temporal points. **An even number of values**
 245 **shall be present, each pair representing one segment.**

246 **BEGIN** range beginning at one temporal point, and extending beyond the end of the acquired data; **a**
 247 **single value shall be present.**

248 **END** a range beginning before the start of the acquired data, and extending to (and including) the
 249 identified temporal point; **a single value shall be present.**

250

251


252 **C.xx.gg.h Referenced Sample Position**

253 *Ed. Note: This is a rewording of existing C.10.10.1.3. In the current Standard this section only belongs to*
 254 *the Waveform Annotation Module*

255 Referenced Sample Positions (0040,A132) may be used only if Referenced Waveform Channels
 256 (0040,A0B0) **in the enclosing dataset** refers to channels within a single multiplex group. The sample
 257 position is by channel, and applies to all channels specified in Referenced Channels (0040,A0B0) **in the**
 258 **enclosing dataset.**

259

260 *Amend Figure F.4.1. Basic Directory IOD Information Model by adding a Waveform Presentation DR*

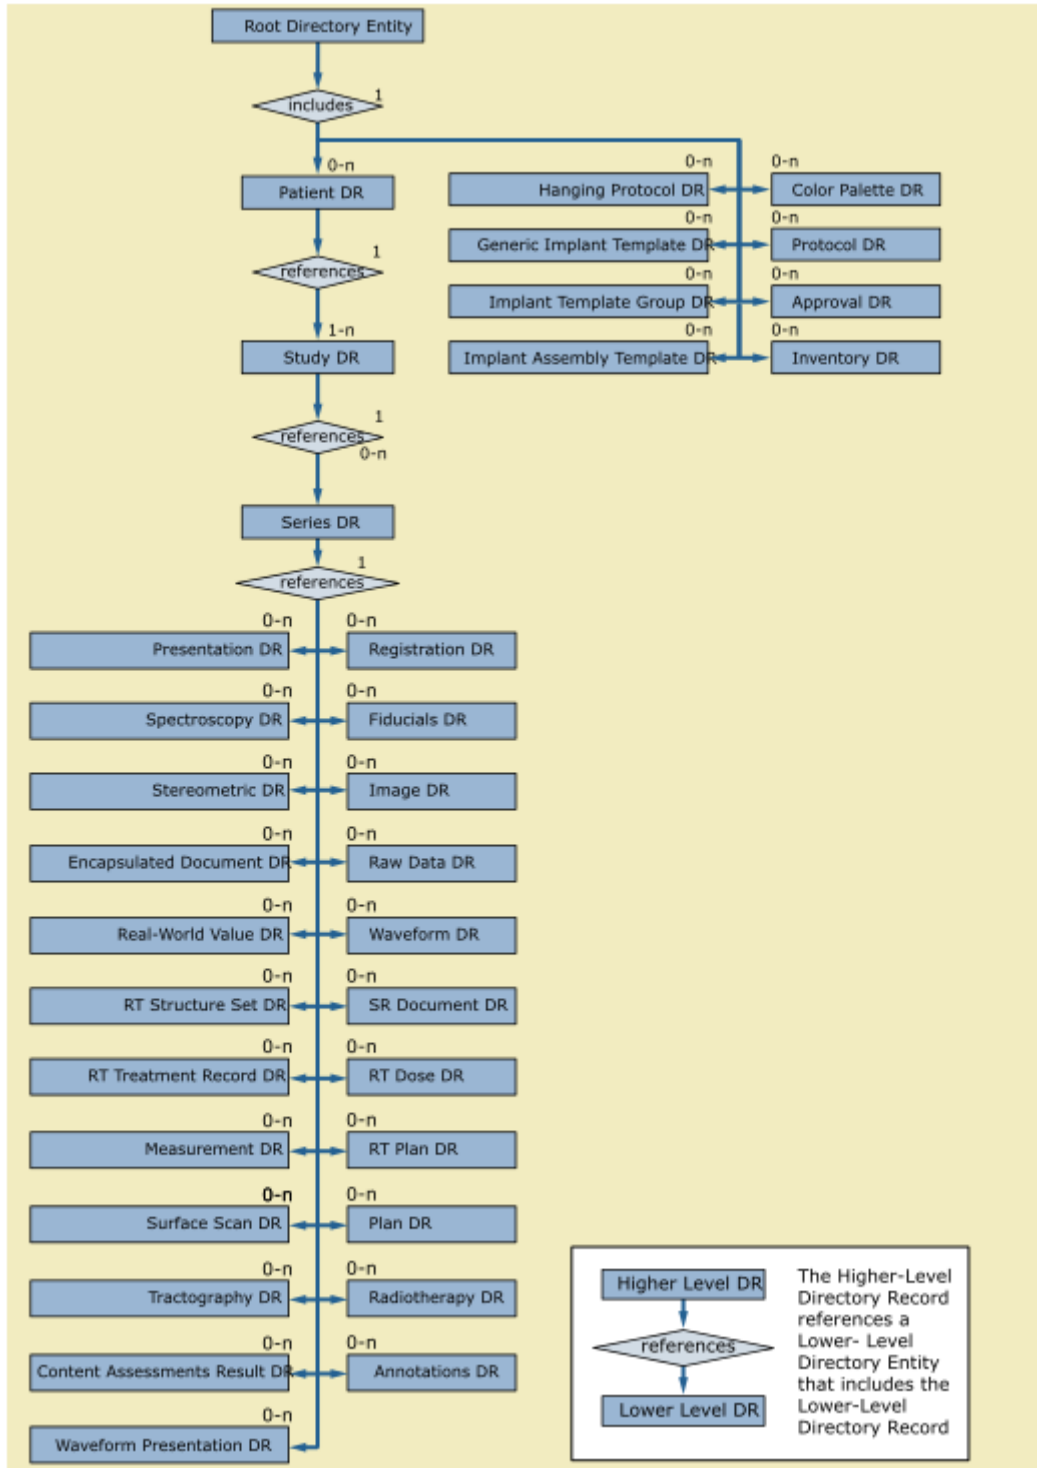

261

262 Add new Basic Directory Record Type to Table F.4-1. Relationship Between Directory Records

263

Table F.4-1. Relationship Between Directory Records

Directory Record Type	Section	Directory Record Types that may be included in the next lower-level directory Entity
...		

WAVEFORM PRESENTATION	F.5.x	PRIVATE

264

265 *Add new Basic Directory Record PS3 Section F.5*

266 **F.5.x Waveform Presentation State Directory Record Definition**

267 The Directory Record is based on the specification of Section F.3. It is identified by a Directory Record
 268 Type (0004,1430) of Value "WAVEFORM PRESENTATION". Table F.5-X lists the set of Keys with their
 269 associated Types for such a Directory Record Type. The description of these Keys may be found in the
 270 Modules related to the Waveform Presentation State IE of Waveform Presentation State IODs. This
 271 Directory Record shall be used to reference a Waveform Presentation State SOP Instance. This Type of
 272 Directory Record may reference a Lower-Level Directory Entity that includes one or more Directory
 273 Records as defined in Table F.4-1

274

275 **Table F.5-X. Waveform Presentation Keys**

Key	Tag	Type	Attribute Description
Specific Character Set	(0008,0005)	1C	Required if an extended or replacement character set is used in one of the Keys.
Presentation Creation Date	(0070,0082)	1	Date on which the waveform presentation was created. Note This date may be different from the date that the DICOM SOP Instance was created, since the presentation information contained may have been recorded earlier.
Presentation Creation Time	(0070, 0083)	1	Time at which this waveform presentation was created. Note: This time may be different from the time that the DICOM SOP Instance was created, since the presentation information contained may have been recorded earlier.
<i>Include Table 10-12 "Content Identification Macro Attributes"</i>			
Referenced Series Sequence	(0008,1115)	1C	Sequence of Items where each Item includes the Attributes of one Series to which the Waveform Presentation State applies. One or more Items shall be included in

			<p>this Sequence.</p> <p>Required if the IOD of the Waveform Presentation State SOP Instance referenced by this Directory Record includes the Waveform Presentation State Relationship Module.</p>
>Series Instance UID	(0020,000E)	1	<p>Unique identifier of a Series that is part of the Study defined by the Study Instance UID (0020,000D) in the enclosing data set.</p> <p>Note The Study Instance UID (0020,000D) value will be that of the Waveform Presentation State.</p>
>Referenced Instance Sequence	(0008,114A)	1C	<p>The set of SR documents containing waveform Annotations to which the Waveform Presentation State applies. These shall be of the Study defined by Study Instance UID (0020,000D) and the Series defined by Series Instance UID (0020,000E).</p> <p>The referenced Instances shall be of SOP Class 1.2.840.10008.5.1.4.1.1.88.77 Waveform Annotation SR Storage.</p> <p>One or more Items shall be included in this Sequence.</p> <p>Required if Structured Waveform Annotation Sequence (ggga,eee1) is present.</p>
>> <i>Include Table 10-11 "SOP Instance Reference Macro Attributes"</i>			
>Referenced Waveform Sequence	(0008,113A)	1	<p>The set of waveforms to which the Waveform Presentation State applies. These shall be of the Study defined by Study Instance UID (0020,000D) and the Series defined by Series Instance UID (0020,000E).</p> <p>One or more Items shall be included in this Sequence.</p> <p>The referenced SOP Class shall be the same for all SOP Instances in a single Item of this Referenced Series Sequence (0008,1115) but may be different for different Items.</p> <p>Notes: 1. For example, some Series might represent EEG and some</p>

			Series might represent ECG. 2. The Presentation State applies to waveforms that are referenced in annotations in Structured Waveform Annotation Sequence (ggga,eee1), thus those waveforms also need to be included here.
>>Include Table 10-11 "SOP Instance Reference Macro Attributes"			
Any other Attribute of the Waveform Presentation State IE Modules		3	

276

Changes to NEMA Standards Publications PS 3.4

277

278

Digital Imaging and Communications in Medicine (DICOM)

279

Part 4: Service Class Specifications

280

281 Add new SOP Class to PS3.4 Annex B tables

B.5 Standard SOP classes

282

283 The SOP Classes in the Storage Service Class identify the Composite IODs to be stored. Table B.5-1
284 identifies Standard SOP Classes.

285 **Table B.5-1. Standard SOP Classes**

SOP Class Name	SOP Class UID	IOD Specification (defined in PS3.3)	Specialization
...			
<u>1.2.840.10008.1.XX1</u>	<u>Waveform Presentation State Storage</u>	<u>Waveform Presentation State IOD</u>	
<u>1.2.840.10008.1.XX2</u>	<u>Waveform Acquisition Presentation State Storage</u>	<u>Waveform Acquisition Presentation State IOD</u>	

286

Changes to NEMA Standards Publications PS 3.6

287

288

Digital Imaging and Communications in Medicine (DICOM)

289

Part 6: Data Dictionary

290

291 Add new Elements to PS3.6 6 Table 6-1. Registry of Data Elements

292

Table 6-1. Registry of DICOM Data Elements

Tag	Name	Keywords	VR	VM	
...					
(ggga,eee1)	Structured Waveform Annotation Sequence	StructuredWaveformAnnotationSequence	SQ	1	
(ggga,eee2)	Waveform Annotation Display Selection Sequence	WaveformAnnotationDisplaySelectionSequence	SQ	1	
(ggga,eeec)	Referenced Montage Index	ReferencedMontageIndex	US	1	
(gggb,eee1)	Waveform Annotation Sequence	WaveformAnnotationSequence	SQ	1	
(gggb,eee2)	Annotation DateTime	AnnotationDateTime	DT	1	
(gggc,eee1)	Displayed Waveform Segment Sequence	DisplayedWaveformSegmentSequence	SQ	1	
(gggc,eee2)	Segment Definition DateTime	SegmentDefinitionDateTime	DT	1	
(gggd,eeea)	Montage Activation Sequence	MontageActivationSequence	SQ	1	
(gggd,eeeb)	Montage Activation Time Offset	MontageActivationTimeOffset	DS	1	
(ggge,eeea)	Waveform Montage Sequence	WaveformMontageSequence	SQ	1	
(ggge,eeeb)	Referenced Montage Channel Number	ReferencedMontageChannelNumber	IS	1	
(ggge,eeec)	Montage Name	MontageName	LT	1	
(ggge,eeee)	Montage Index	MontageIndex	US	1	
(ggge,eeed)	Montage Channel Sequence	MontageChannelSequence	SQ	1	
(gggf,0202)	Montage Channel Number	MontageChannelNumber	IS	1	
(gggf,0203)	Montage Channel Label	MontageChannelLabel	SH	1	
(gggf,0208)	Montage Channel Source Sequence	MontageChannelSourceSequence	SQ	1	
(gggf,0209)	Contributing Channel Sources Sequence	ContributingChannelSourcesSequence	SQ	1	
(gggf,020A)	Calculatory Weight	CalculatoryWeight	FL	1	
(gggf,020B)	Contributing Channel Source Sequence	ContributingChannelSourceSequence	SQ	1	
..					

293
294

295 *Add new SOP Classes to PS3.6 Annex A Table A-1:*

296

UID Value	UID Name	UID Keyword	UID Type	Part
-----------	----------	-------------	----------	------

...				
<u>1.2.840.10008.1.XX1</u>	<u>Waveform Presentation State Storage</u>	<u>WaveformPresentation StateStorage</u>	<u>SOP Class</u>	<u>PS3.4</u>
<u>1.2.840.10008.1.XX2</u>	<u>Waveform Acquisition Presentation State Storage</u>	<u>WaveformAcquisitionPr esentationStateStorage</u>	<u>SOP Class</u>	<u>PS3.4</u>
...				

297

298

299

300

301

302
303
304
305

Changes to NEMA Standards Publications PS3.15
Digital Imaging and Communications in Medicine (DICOM)
Part 15: Security and System Management Profiles

306 *Add the new Modules from the new IODs to PS3.15 Section C.2 by continuation of the list*

307 ...

308 As a minimum, an implementation shall include the following Attributes in generating the Creator RSA Digital
309 Signature:

310 a. the SOP Class and Instance UIDs

311 b. the SOP Creation Date and Time, if present

312 c. the Study and Series Instance UIDs

313 d.

314 **ae. any Attributes of the Waveform Presentation State Relationship Module that are present**

315 **af. any Attributes of the Structured Waveform Annotation Module that are present**

316 **ag. any Attributes of the Simple Waveform Annotation Module that are present**

317 **ah. any Attributes of the Displayed Waveform Segment Module that are present**

318 **ai. any Attributes of the Montage Activation Module that are present**

319 **aj. any Attributes of the Waveform Presentation Montage Module that are present**

320 *Add new Data Elements to PS3.15 Annex E*

321

Table E.1-1. Application Level Confidentiality Profile Attributes

Attribute Name	Tag	Retd. (from PS3.6)	In Std. Comp. IOD (from PS3.3)	Basic Prof.	Rtn. Safe Priv. Opt.	Rtn. UIDs Opt.	Rtn. Dev. Id. Opt.	Rtn. Inst. Id. Opt.	Rtn. Pat. Chars. Opt.	Rtn. Long. Full Dates Opt.	Rtn. Long. Modif. Dates Opt.	Clean Desc. Opt.	Clean Struct. Cont. Opt.	Clean Graph. Opt.
...														
<u>Annotation DateTime</u>	<u>(gggb.eee2)</u>	<u>N</u>	<u>Y</u>	<u>X/Z</u>						<u>K</u>	<u>C</u>			
<u>Segment Definition DateTime</u>	<u>(gggc.eee2)</u>	<u>N</u>	<u>Y</u>	<u>X/Z</u>						<u>K</u>	<u>C</u>			
...														

322

323

324 **Changes to NEMA Standards Publications PS3.17**
325
326 **Digital Imaging and Communications in Medicine (DICOM)**
327 **Part 17: Explanatory Information**

328 **XXX Waveform Presentation (Informative)**

329
330 In clinical neurophysiology it is important to be able to recreate the presentation of the recorded data as it
331 was displayed during the recording or during review and reporting. This allows subsequent reviewers to
332 recreate the display when an annotation was created, for example to review subtle features that may not
333 be obvious in other channel montages or reference states.

334 In cardiology, technicians annotate previously recorded waveforms (e.g. from home monitoring Holter
335 ECG) and highlight areas of interest. This information is essential input for the cardiologist who reviews
336 the ECG and finally provides the report.

337 Waveform objects support limited display information, which has to be provided within the recorded
338 waveform objects. These Attributes only cover color and scaling of waveform channels.

339 In neurophysiology a **montage** defines a list of channels for visualization of the data which is created
340 from the originally recorded channel sources and it conveys the method for their mathematical (linear)
341 recombination. In principle montages could be either predefined and referenced by an object identifier or
342 defined for each specific recording.

343 **Waveform Annotations** are textual or coded markers assigned to a specific timepoint or time range,
344 related to all channels or a selected set of channels. Annotations could be observations of waveforms,
345 patient stimuli, comments about the recording, as well as measurements.

346 A **Waveform Presentation State Object** stores annotations, filters, and montages used for a given
347 recording (patient related). A Waveform Presentation State object is stored together with the waveform
348 study (e.g. a Routine Scalp EEG recording) and can be exchanged between systems.

349
350 **Use case: Recording**

351 A technician performs an EEG recording. From time to time he changes the filter settings and also the
352 montages, for example to check the quality of the raw channel data. If abnormalities occur or if external
353 circumstances change that could be of importance for the evaluation of the recording, the technician adds
354 an annotation at this point.

355 In addition to the annotations, the recording system also saves the current filter settings and the montage
356 selected for the display in a waveform presentation state object.

357
358 **Use case: Post-hoc Review**

359 A physician acting as a post-hoc reviewer looks through a completed EEG recording and marks potential
360 epileptiform features. The annotations added by the technician during the recording are displayed for
361 anyone reviewing the recording. The reviewing physician has the option of using the settings for display
362 filters and montage stored in the presentation state object generated during recording.
363 If he adds annotations, these are stored as well.

364
365 **Use case: Electronic Health Record**

366 An epilepsy patient is treated in another organization and the neurologist wants to see the EEGs and
367 findings of previous epilepsy monitoring recordings (accessible via the patient's health record). Montages
368 and filter settings used during recording and review may be different between hospitals, and the
369 neurologist may need to see directly what the outside EEG staff annotated, or she may wish to review the
370 data with montage settings she prefers.

371
372 **Use case: Automated Waveform Analysis**

373 Algorithms may store observations and measurements as annotations and the settings used by the
374 algorithm in the recorded data for future reference.

375 All these use cases require time locked annotations with identification of authorship and situation of
376 annotation ('during acquisition' versus 'post hoc')

377